

Recommended Installation

When possible, the EOGas 4 Sterilizer

should be located near an outside wall,

and exhaust directly to the outside by

means of ³/₄" (1.9cm) I.D. tubing.

Through-wall mounting kits are

Note: Sterilizer must be placed

in an area that can maintain

Alternate Option 1

Quick release connector

available from Andersen.

68°F or above room

temperature.

Installation Guidelines EOGas 4 sterilizer installation options

Exterior*

Exterior*

Wall

Quick

release

connector

Exterior*

Remote location installation

damage.)

materials.

The $\frac{3}{4}$ " (1.9cm) I.D. braided tubing may be

up to 200' (60.96m) in length allowing for sterilizer placement in remote locations.

(Choose a path that will provide exhaust tubing protection from obstruction or

Note: Installation in plenum designated


areas require use of plenum rated

Ouick

release

connector



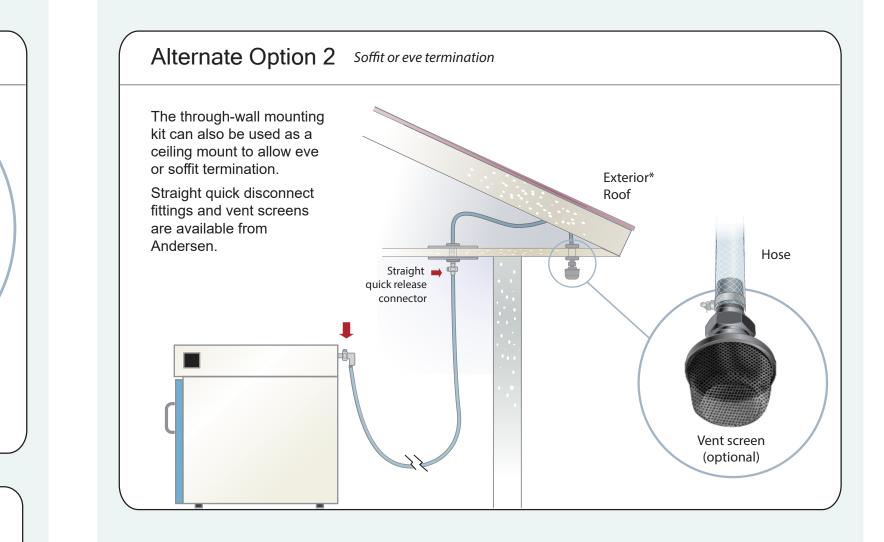

* Please note: AAMI guidelines recommend all EO sterilizers be vented through a dedicated exhaut line to the outside atmosphere directly or through an emission control system. The vent should not terminate within 25 feet of any building air intake source or near pedestrian or animal traffic, nor should it allow EO release into or to reenter the building.

For further installation assistance please call your Andersen representative or 1.800.523.1276



Andersen Products, Inc. Health Science Park • 3202 Caroline Drive Haw River, NC 27258-9564 USA 800.523.1276





Installation Guidelines





Distributed in Europe by: H.W. Andersen SARL Distributed in UK, Australia, Africa & Middle East b H.W. Andersen Products. Ltd