



Installation Guidelines EOGas 4 sterilizer installation options


Recommended Installation When possible, the EOGas 4 Sterilizer Quick should be located near an outside wall, release connector and exhaust directly to the outside by Exterior* means of 3/4" (1.9cm) I.D. tubing. Through wall mounting kits are available from Andersen. Note: Sterilizer must be placed in an area that can maintain 68°F or above room temperature. Exterior* Quick release connector



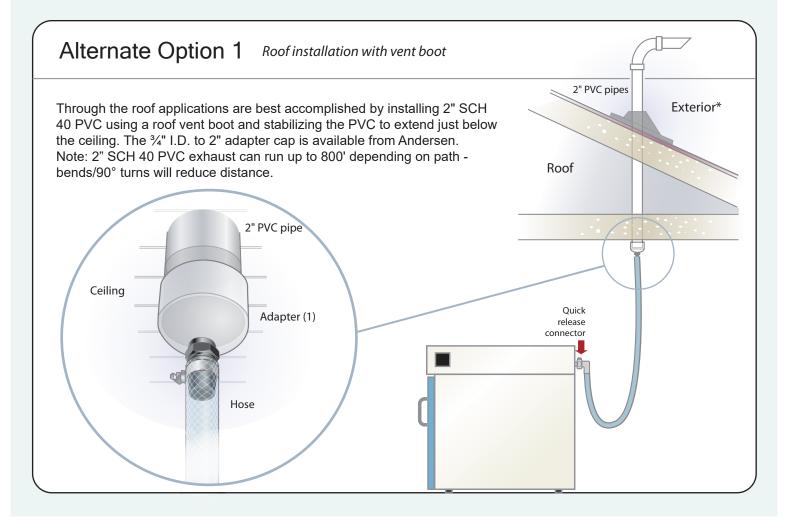

Installation Guidelines

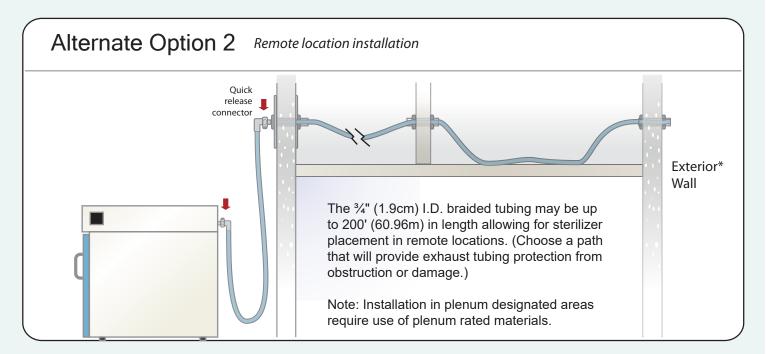

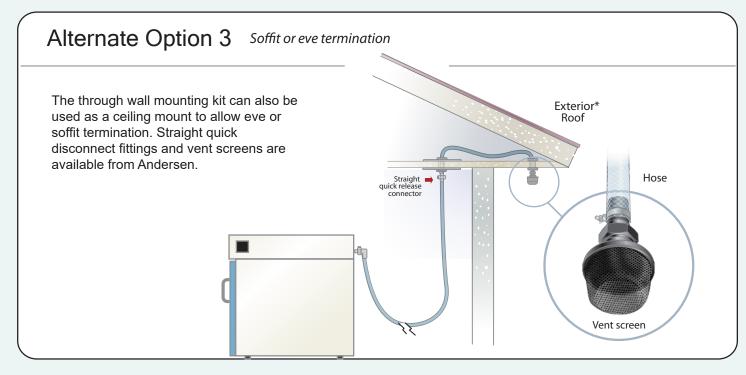

* Please note: AAMI guidelines recommend all EO sterilizers be vented through a dedicated exhaut line to the outside atmosphere directly or through an emission control system. The vent should not terminate within 25 feet of any building air intake source or near pedestrian or animal traffic, nor should it allow EO release into or to reenter the building

For further installation assistance please call your Andersen representative or 1.800.523.1276

sterility.com

Join Us: Follow, Like, Share















Health Science Park • 3202 Caroline Drive



